


SN# 18062001 Lamp Specific Acceptance Test




Model: UV-4000, Profusion	Result	Steady State	Acceptable	Units
Peak Output Wavelength	Pass	370 $\checkmark$	365 ± 5	nm
Full Width Half Maximum (FWHM)	Pass	10 $\checkmark$	≤ 15	nm
Full Width at 10% Maximum	Pass	22 $\checkmark$	≤ 30	nm
Longest Wavelength at Half Maximum	Pass	375 $\checkmark$	≤ 377	nm
Max Excitation Irradiance (347-382 nm)	Pass	3939 $\checkmark$	≥ 2000	$\mu\text{W}/\text{cm}^2$

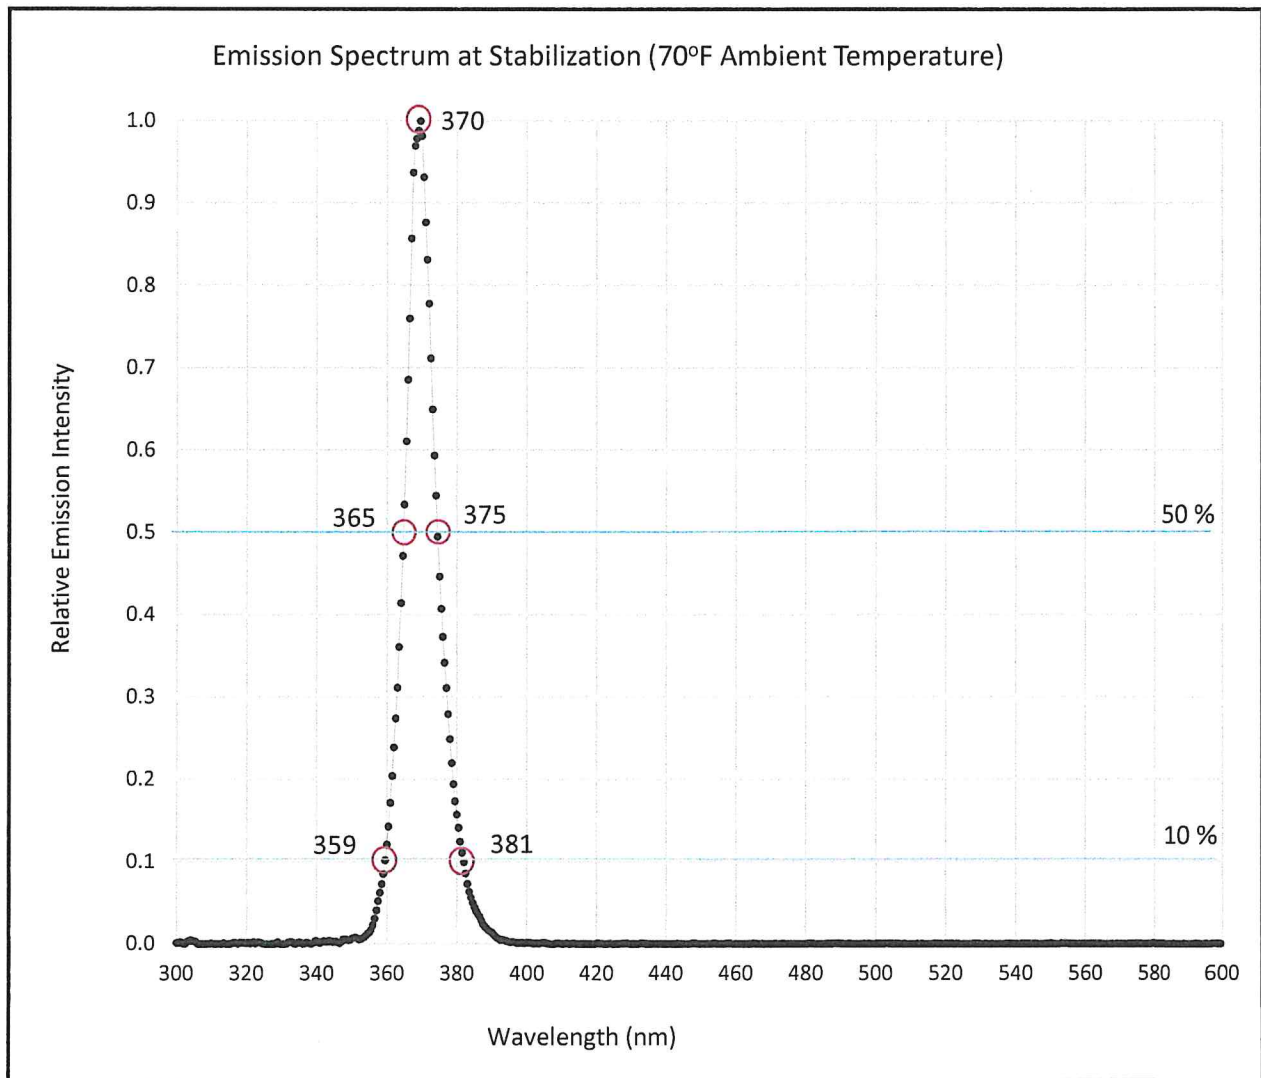

Inspector: REL INC MK
 Date of Certification: 4.15.2026

This lamp has been tested to conform to all requirements of:
 ASTM E3022 $\checkmark$ AITM6-1001 $\checkmark$ ISO 3059 $\checkmark$ RRES 90061 $\checkmark$

Emission Spectrum Measured at Stabilization Temperature with Blue-wave UV-25 S/N 18120729, Certificate Number 18120729-UV-CR2-0925

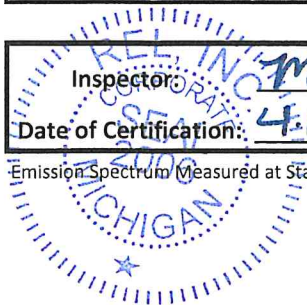

Profusion Series, Certificate of Conformance



SN# 18062001_profusion_recert1	Switch On	Steady State	Elevated Temp*	Acceptable	Units
Peak Output Wavelength	369	370	370	365 ± 5	nm
Full Width Half Maximum (FWHM)	10	10	13	≤ 15	nm
Full Width at 10% Maximum	22	22	26	≤ 30	nm
Longest Wavelength at Half Maximum	374	375	377	≤ 377	nm
Visible Emission at 15 in	14	13	10	≤ 20	Lux
Visible Emission at 36 in	3	3	3	≤ 5	Lux
Irradiated Area at 15 in (>1000 μW/cm ²)	11	10	9	≥ 5	Inch Diameter
Max Excitation Irradiance (347-382 nm)	4,608	3,939	2,400	≥ 2,000	μW/cm ²
Irradiance at Peak Output Wavelength	406	347	185	-	μW/cm ²
Min Working Distance** (< 5000 μW/cm ²)	15	14	13	-	Inches
Max Working Distance** (> 1200 μW/cm ²)	25	21	19	-	Inches
Body Stabilization Temp (70°F Ambient)	-	104	-	≤ 120	°F
Current Ripple	9	9	9	≤ 35	mA peak-peak

* Tested in a 115° F Environment, the maximum ambient temperature where light still meets all requirements

** Profusion series lights use a single LED emitter, thus beam uniformity does not change with working distance (RRES 90061)

