SN# 19121019 Lamp Specific Acceptance Test

Model: UV-4000, Profusion	Result	Steady State	Acceptable	Units
Peak Output Wavelength	Pass	369	365 ± 5	nm
Full Width Half Maximum (FWHM)	Pass	11	≤ 15	nm
Full Width at 10% Maximum	Pass	23	≤ 30	nm
Longest Wavelength at Half Maximum	Pass	375	≤ 377	nm
Max Excitation Irradiance (347-382 nm)	Pass	3879	≥ 2000	$\mu W/cm^2$

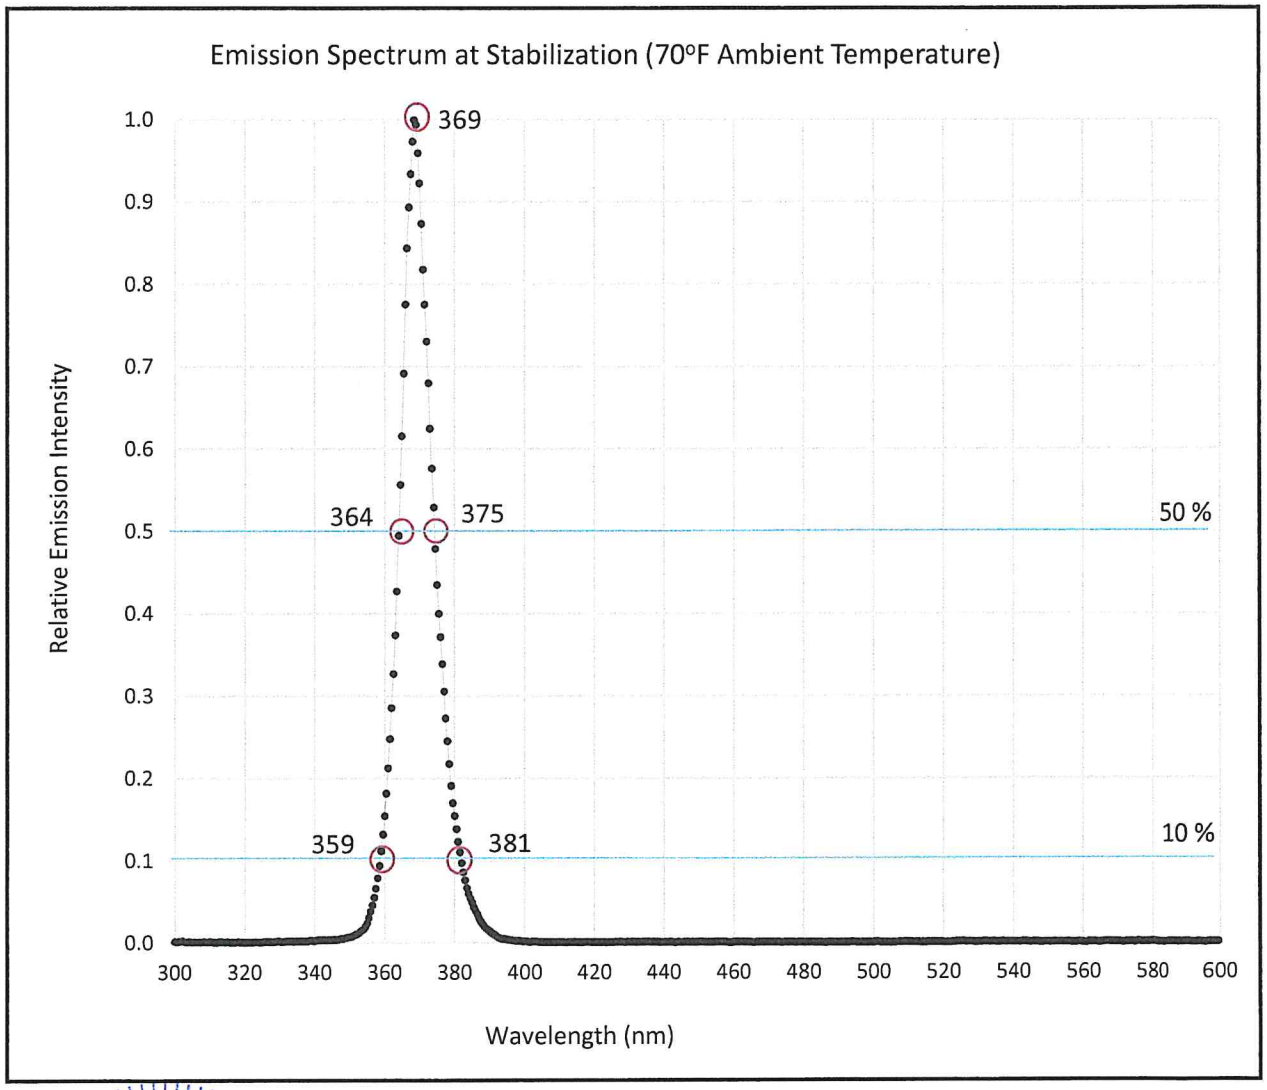

Inspector: MK

Date of Certification: 10-1-2026

This lamp has been tested to conform to all requirements of:

ASTM E3022 ✓ AITM6-1001 ✓ ISO 3059 ✓ RRES 90061 ✓

Emission Spectrum Measured at Stabilization Temperature with Blue-wave UV-25 S/N 26011309, Certificate Number 26011309-UV-CR2-0126

Profusion Series, Certificate of Conformance

SN# 19121019_profusion_recert1	Switch On	Steady State	Elevated Temp*	Acceptable	Units
Peak Output Wavelength	368	369	370	365 ± 5	nm
Full Width Half Maximum (FWHM)	11	11	13	≤ 15	nm
Full Width at 10% Maximum	23	23	26	≤ 30	nm
Longest Wavelength at Half Maximum	374	375	377	≤ 377	nm
Visible Emission at 15 in	14	13	10	≤ 20	Lux
Visible Emission at 36 in	3	3	3	≤ 5	Lux
Irradiated Area at 15 in (>1000 µW/cm^2)	11	10	9	≥ 5	Inch Diameter
Max Excitation Irradiance (347-382 nm)	4,539	3,879	2,400	≥ 2,000	µW/cm^2
Irradiance at Peak Output Wavelength	388	332	185	-	µW/cm^2
Min Working Distance** (< 5000 µW/cm^2)	15	14	13	-	Inches
Max Working Distance** (> 1200 µW/cm^2)	25	21	19	-	Inches
Body Stabilization Temp (70°F Ambient)	-	104	-	≤ 120	°F
Current Ripple	9	9	9	≤ 35	mA peak-peak

** Tested in a **115° F** Environment, the **maximum ambient temperature where light still meets all requirements***

*** Profusion series lights use a single LED emitter, thus beam uniformity does not change with working distance (RRES 90061)*

